
ADC® Advantage™ Automatic Blood Pressure Monitor

6015N, 6016N

Instructions for Use



ADC® Advantage™ Automatic Blood Pressure Monitor
Table of Contents

I. A Special Thank You	4
1. INTRODUCTION AND INTENDED USE	4
2. WARNINGS AND PRECAUTIONS	5
3. ABOUT BLOOD PRESSURE	6
3.1. What Is Blood Pressure?	6
3.2. What Is a Normal Blood Pressure?	6
3.3. What Influences Blood Pressure?	7
3.4. Does Blood Pressure Vary?	7
3.5. What Is Hypertension?	7
3.6. Can Hypertension Be Controlled?	8
3.7. Why Measure Blood Pressure at Home?	8
3.8. How Is Blood Pressure Measured?	9
3.9. How Should I Record My Blood Pressure?	9
4. COMPONENTS OF YOUR BLOOD PRESSURE MONITOR	10
5. SETTING UP YOUR BLOOD PRESSURE MONITOR	11
5.1. Inserting the Batteries	11
5.2. Setting the Time and Date	11
5.3. Selecting the User	12
5.4. Selecting the Measurement Mode	12
5.5. Using ADC Average Mode Technology (6016N only)	12
6. MEASUREMENT PROCEDURE	13
6.1. Before Measurement	13
6.2. Common Sources of Error	13
6.3. Fitting the Cuff	14
6.4. Measurement Procedure	14
6.5. Discontinuing a Measurement	15
6.6. Reading Measurement Results	15

7. SOFTWARE FUNCTIONS	16
7.1. PC Link Installation and Data Transmission (6016N only)	16
7.2. Installing and Using Microsoft HealthVault	17
8. IRREGULAR HEARTBEAT DETECTOR	18
8.1. Traffic Light Indicator (6016N only)	18
9. MEMORY FUNCTION	19
9.1. Recall and Storage of Measurements	19
9.2. Delete Memory	19
10. ERROR MESSAGES/TROUBLESHOOTING	19
11. CARE AND MAINTENANCE	21
12. TECHNICAL SPECIFICATIONS	22
13. WARRANTY	23
14. QUALITY STANDARDS	23
15. SYMBOL DEFINITIONS	23
16. HOW TO CONTACT US	24

I. A Special Thank You

Congratulations on your purchase of an ADC® Advantage™ Automatic Blood Pressure Monitor.

In hospitals and physician's offices throughout the world, where accuracy and dependability are critical, ADC professional diagnostic products are the instruments of choice.

Now you, too, can enjoy the benefits of ADC engineering and quality in the home. This feature rich instrument was designed to simplify the measurement of blood pressure and pulse rate at home and deliver consistent, dependable results.

Read this booklet thoroughly before attempting to use your new ADC Advantage Automatic Blood Pressure Monitor.

1. INTRODUCTION AND INTENDED USE

This manual is for Advantage 6015N and Advantage Ultra 6016N. To find the model number of your device, look on the rating label located on the cuff.

Your monitor is a fully automatic, digital blood pressure measuring device for use on the wrist. Features include irregular heartbeat detection, average mode (6016N model only), and PC Link blood pressure analyzer software (6016N model only). This monitor enables fast and reliable measurement of your systolic and diastolic blood pressure as well as pulse by way of the oscillometric measurement method. It's clinically tested for measurement accuracy and designed for maximum user-friendliness.

Before using, please read this instruction manual carefully and then keep it in a safe place. Please contact your doctor for further questions on the subject of blood pressure and its measurement.

To learn more, visit our website at: www.adctoday.com.

Remember...

- Only a healthcare professional is qualified to interpret blood pressure measurements. This device is NOT intended to replace regular medical checkups.
- It is recommended that your physician review your procedure for using this device.
- Blood pressure readings obtained by this device should be verified before prescribing or adjusting any medications used to control hypertension. Under no circumstances should YOU alter the dosages of any drugs prescribed by your doctor.
- This monitor is intended for use by adults only. Consult with a physician before using this instrument on a child.
- In cases of irregular heartbeat (arrhythmia), measurements made with this instrument should only be evaluated after consultation with your doctor.
- Familiarize yourself with the section titled "About Blood Pressure." It contains important information on the dynamics of blood pressure readings and will help you to obtain the best results.

2. WARNINGS AND PRECAUTIONS

Warning: The device contains sensitive electronic components. Avoid strong electrical or electromagnetic fields in the direct vicinity of the device (e.g., mobile telephones, microwave ovens). These can lead to temporary impairment of the measuring accuracy.

Warning: Use of this instrument on patients under dialysis therapy or on anticoagulant, antiplatelets, or steroids could cause internal bleeding.

Warning: Do not use cuffs or batteries other than those included with this product or replacement parts supplied by the manufacturer.

Warning: This system may fail to yield specified measurement accuracy if operated or stored in temperature or humidity conditions outside the limits stated in the specifications section of this manual.

Caution: The standard material used is made without natural rubber latex or phthalates.

Attention: Self-measurement means control, not diagnosis or treatment. Unusual values must always be discussed with your doctor. Under no circumstances should you alter the dosages of any drugs prescribed by your doctor.

Attention: The pulse display is not suitable for checking the frequency of heart pacemakers!

Attention: In cases of irregular heartbeat, measurements made with this instrument should only be evaluated after consultation with your doctor.

NOTE: To obtain the greatest accuracy from your blood pressure instrument, it is recommended that the instrument be used within a temperature range of 50°F (10°C) to 104°F (40°C), with a 15-90% relative humidity.

3. ABOUT BLOOD PRESSURE

3.1. What is Blood Pressure?

Simply put, arterial blood pressure is the force of blood exerted against the walls of the arteries. There are two components to blood pressure: systolic and diastolic pressure. Systolic, the higher pressure, occurs during contraction of the heart. Diastolic, the lower pressure, occurs when the heart is at "rest."

Your level of blood pressure is determined in the circulatory center of the brain and adjusts to a variety of situations through feedback from the nervous system. To adjust blood pressure, the strength and frequency of the heart (pulse), as well as the width of circulatory blood vessels is altered. Blood vessel width is affected by fine muscles in the blood vessel walls. Blood pressure is traditionally measured in millimeters of mercury (mmHg).

It is recorded as systolic/diastolic. For example a systolic of 120 and diastolic of 80 would be recorded 120/80.

Blood pressure is a dynamic vital sign, one that changes constantly throughout the day. A person's "resting" blood pressure is the pressure that exists first thing in the morning while a person is still at rest and before consumption of food or drink.

3.2. What Is a Normal Blood Pressure?

A systolic pressure of less than 120mmHg and a diastolic pressure of under 80mmHg are recognized as normal by the Joint National Committee on Prevention, Detection, Evaluation, and Treatment of High Blood Pressure, 2003.

NOTE: Blood pressure does increase with age, so you must check with your doctor to find out what is "normal" for you! Even with normal blood pressure values, a regular self-check with your blood pressure monitor is recommended. You can detect possible changes in your values early and react appropriately. If you are undergoing medical treatment to control your blood pressure, keep a record of values along with time of day and date. Show these values to your doctor. Never use the results of your measurements to independently alter the drug doses prescribed by your doctor.

3.3. What Influences Blood Pressure?

Blood pressure is influenced by many factors including age, weight, physical conditioning, past illness, time of day, altitude, activity, and climate, to name just a few. In general, blood pressure is lower in the morning and increases throughout the day. It is lower in warm weather, and higher in cold weather.


Physical activity can have a significant short term impact on blood pressure. Work, exercise, smoking, eating, drinking - even talking, laughing, or crying - will all affect a person's blood pressure.

Your diet, including beverages containing caffeine or alcohol, may affect blood pressure. Emotional stress can have a dramatic impact on your blood pressure.

Even repeated blood pressure measurements taken without adequate rest between readings will alter your blood pressure as the vessels in your arm engorge with blood. Many of these influences are only temporary or short term, though chronic (long term) exposure to some factors may result in permanently elevated blood pressure levels.

3.4. Does Blood Pressure Vary?

Constantly. An individual's blood pressure varies greatly on a daily and seasonal basis. It changes throughout one's lifetime. It is not uncommon for systolic pressure to vary by 40mmHg or more throughout the course of a single day!

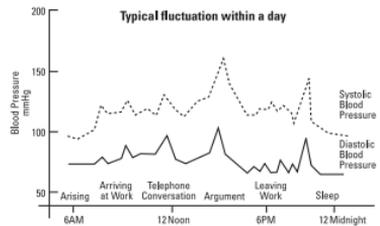

While generally not as volatile, diastolic pressure can still vary significantly. In hypertensive individuals, variations are even more pronounced. Normally, blood pressure is at its lowest during sleep and rises in the morning and throughout the day. The chart (right) illustrates the fluctuations that could occur in a typical day.

3.5. What Is Hypertension?

Hypertension (high blood pressure) is elevated systolic or diastolic levels. In 90 to 95 percent of the diagnosed cases, the specific causes are unknown, although the condition is often linked with family history and lifestyle. This is referred to as essential hypertension. In the remaining cases, high blood pressure is a symptom of an underlying, often treatable condition, which if corrected, may normalize blood pressure. This less common type is known as secondary hypertension. Hypertension, if left untreated, may contribute to kidney disease, heart attack, stroke, or other debilitating illnesses. The following standards for assessment of high blood pressure in adults have been established by the Joint National Committee, 2003.

Range Classifications	Systolic Blood Pressure	Diastolic Blood Pressure	Precaution Measures
Normal	<120	<80	Monitor regularly
Prehypertension	120 - 139	80 - 89	Contact your physician
HYPERTENSION			
Stage 1 (Moderate)	140 - 159	90 - 99	Contact your physician Immediately
Stage 2 (Severe)	≥160	≥100	Contact your physician URGENTLY

(JNC-7 report: Joint National Committee on Prevention, Detection, Evaluation and Treatment of High Blood Pressure / 2003)

Remember, only a physician is qualified to interpret the readings obtained from your blood pressure monitor. No attempt should ever be made at self-diagnosis or treatment.

3.6. Can Hypertension Be Controlled?

Although essential hypertension cannot be cured, it can usually be controlled by altering your lifestyle. Including diet, adopting a program of exercise and stress management and, where necessary, with medication under a doctor's supervision.

To help reduce the risk of hypertension, or keep it under control, the American Heart Association (AHA) recommends the following:

- Don't smoke
- Reduce salt and fat intake
- Maintain proper weight
- Exercise regularly
- Have regular physical checkups

3.7. Why Measure Blood Pressure at Home?

Clinical studies have shown improved detection and treatment of hypertension when regular home blood pressure monitoring is done in consultation with a physician.

Blood pressure measured in a doctor's office or hospital setting may cause anxiety and lead to an elevated reading—a condition referred to as "white coat hypertension."

Home measurements generally reduce the "outside" influences on blood pressure readings, and can provide a more comprehensive and meaningful blood pressure history.

Note: While it is important to keep an accurate record of your blood pressure measurements, don't be overly concerned by the results of any one measurement. Individual results may be influenced by spiking of your pressure due to diet or anxiety, or mis-

measurement resulting from excessive arm movement or misapplication of the cuff. Many readings taken at the same time each day give a more comprehensive blood pressure history.

Always be sure to note the date and time when recording blood pressure and pulse measurements. For best results, and with time permitting, three successive measurements may be taken daily.

Make sure to allow at least one minute between measurements. Discard any reading that appears suspect and record the average of the remaining readings.

3.8. How Is Blood Pressure Measured?

Healthcare professionals traditionally use a device known as a sphygmomanometer along with a stethoscope - essentially a professional version of the very same instrument you have purchased. The sphygmomanometer is a system consisting of an inflatable bladder contained within a cuff, inflation bulb with air control valve, and pressure measuring manometer (gauge). The gauge may be mechanical, electronic, or mercurial. The cuff is wrapped around the limb and inflated to constrict blood flow to the artery. As pressure is released from the cuff through the deflation valve, blood flow returns to the artery producing pulse beats known as Korotkoff sounds, which are detected with the stethoscope. Systolic pressure is recorded at the onset of these sounds. Diastolic pressure is generally recorded when the sounds disappear (when blood flow to the artery returns to normal).

3.9. How Should I Record My Blood Pressure?

Record your blood pressure by setting up a simple chart in a spiralbound notebook as shown below, or use the included record book.

Date	Time	Reading	Pulse
4/24	7:50AM	128/83	72
4/25	8:00AM	135/77	77
4/26	7:45AM	130/75	71
4/27	2:00PM	153/89	80

If you like you can add a column for comments about your condition at the time of measurement, or a listing of any factors that may have influenced your readings (such as "had a cold," or "just returned from vacation").

For best results, and with time permitting, three successive measurements may be taken daily. Make sure to allow at least a one minute interval between measurements.

Discard any reading that appears suspect and record the average of the remaining readings. If this method is used, be sure to note that the readings are averaged.

On the Advantage Ultra (6016N) model, PC Link software is available. Records can be automatically transferred to your Windows computer. Many smart phone and tablet apps allow you to record, chart, and share your BP measurements. ADC recommends Microsoft® Healthvault™.

4. COMPONENTS OF YOUR BLOOD PRESSURE MONITOR

The illustration shows your blood pressure monitor. The unit includes a wrist monitor with attached cuff, storage case, and instruction booklet.



For wrist circumference: 5.3–7.7” (13.5–19.5 cm)

5. SETTING UP YOUR BLOOD PRESSURE MONITOR


5.1. Inserting the batteries

After you have unpacked your device, insert the batteries. The battery compartment is located on the bottom of the device.

- Push and lift to remove the battery cover.
- Insert the batteries (2 x AAA, 1.5V), observing the indicated polarity.

Attention!


- If a battery warning  appears in the display, the batteries are almost discharged and must be replaced.
- After battery warning  appears, the device will not work until the batteries have been replaced.
- If the blood pressure monitor is not used for long periods, remove the batteries from the device.
- Use AAA Long-Life or Alkaline 1.5V batteries. Do not use rechargeable batteries.
- Functional check: Press the «**MEMORY**» button down to test all the display elements. When functioning correctly many icons will appear.



5.2. Setting the Time and Date

This blood-pressure monitor incorporates an integrated clock with date display. After new batteries have been inserted, the device will request the date and time to be reset.

- After new batteries have been inserted, you will have to set the year. The four digits (2014) on the screen will flash. You can advance the year by pressing the «**MEMORY**» button. To confirm and set the year, press the «**TIME**» button.
- To set the month, use the «**MEMORY**» button. To confirm and set the month, press the «**TIME**» button.
- To set the day, use the «**MEMORY**» button. Press the «**TIME**» button to confirm. To set the hour, use the «**MEMORY**» button. Press the «**TIME**» button to confirm.
- To set the minutes, use the «**MEMORY**» button. Press the «**TIME**» button to confirm.
- Once you have set the minutes and pressed the «**TIME**» button, the date and time are set and the time is displayed.



NOTE

- If you want to change the date and time, press and hold the «**TIME**» button down for approx. three seconds until the user icon starts to flash. Press the «**TIME**» button again; now you can enter the new values as described above.
- A single press of the «**MEMORY**» button or «**TIME**» button advances one operation.
- Holding the button down speeds up the procedure.

5.3. Selecting the User

This blood pressure monitor is designed to store 99 measurements for each of two users. Before taking a measurement, be certain that the correct user has been selected.

- a) With the unit off, press and hold the «**TIME**» button to cycle between users ("1" and "2").
- b) Press the «**MEMORY**» button to toggle between users.
- c) Press the «**ON/OFF**» button to make your selection.



5.4. Selecting the Measurement Mode (6016N only)

This instrument enables you to select either standard (single) measurement or averaging mode (automatic triple measurement).

- a) To select Standard mode, push the switch on the side of the instrument to position "1".
- b) To select Averaging mode, push the switch to Position "3."



Note: The MAM Advantage™ Averaging mode icon will illuminate on the display.



If you select 1, then only one measurement will be taken. If you select 3, the unit will inflate and deflate three times resulting in one final average.

5.5. Using ADC Average Mode Technology (6016N only)

1. In MAM Advantage Averaging mode, three measurements are automatically taken in succession and the result then automatically analyzed and displayed. Because your blood pressure constantly fluctuates, a result determined in this way is more reliable than one produced by a single measurement.

2. After pressing the «**ON/OFF**» button, the MAM Advantage Averaging mode  icon appears in the display.
3. The bottom right hand section of the display shows a 1, 2, or 3 to indicate which of the three measurements is currently being taken.
4. There is a break of 15 seconds between the measurements (15 seconds are adequate according to “Blood Pressure Monitoring, 2001, 6:145-147” for oscillometric instruments). A countdown indicates the remaining time.
5. The individual results from measurements 1, 2 and 3 are not initially displayed.

NOTE: If you want to see each of the individual readings making up a triplicate reading, turn the unit off, then press and hold the Memory button for three seconds, until you hear a tone, immediately after a MAM Advantage Averaging Mode measurement. Note: You can only see the individual readings one time immediately following an Averaging Mode measurement.

Do not remove the cuff between measurements.

6. MEASUREMENT PROCEDURE

6.1. Before Measurement:

- Avoid eating and smoking as well as all forms of exertion directly before measurement. These factors influence the measurement result. Find time to relax by sitting in an armchair in a quiet atmosphere for about five minutes before taking a measurement.
- Always measure on the same wrist (normally left).
- Always compare measurements taken at the same time of day, since blood pressure changes during the course of the day, as much as 20-40 mmHg.

6.2. Common Sources of Error:

NOTE: Comparable blood pressure measurements always require the same conditions! Conditions should always be quiet.


- All efforts by the user to support the arm can increase blood pressure. Make sure you are in a comfortable, relaxed position and do not flex any of the muscles in the measurement arm during the measurement. Use a cushion for support if necessary.
- If the arm artery lies considerably lower or higher than the heart, an

erroneously high or low blood pressure will be measured! Each 15cm (6 inch) difference in height between your heart and the cuff results in a measurement error of 10 mmHg!

- A loose cuff or a sideways protruding air pocket causes false measurement values.
- With repeated measurements, blood accumulates in the arm, which can lead to false results. Consecutive blood pressure measurements should be repeated after a one minute pause or after your arm has been held up in order to allow the accumulated blood to flow away. If you decide to take your Averaging Mode measurement again, be sure to wait at least one minute beforehand.

6.3. Fitting the Cuff

- a) Remove all objects and jewelry (e.g., wristwatch) from the wrist in use. Put the cuff over the wrist with the monitor face on the inside of the wrist. The buttons should be on the bottom.
- b) The distance between the cuff and the hand should be approx. 10 mm (1/2").
- c) Secure the cuff with the hook-and-loop fastener, so that it lies comfortably and not too tight. No space should remain between the cuff and the wrist.
- d) Lay your arm on a table, with the palm upwards. Support the arm a little with a cushion, so that the cuff rests at about the same height as the heart. Remain still for two minutes before beginning the measurement. You can also use the storage case as a support.

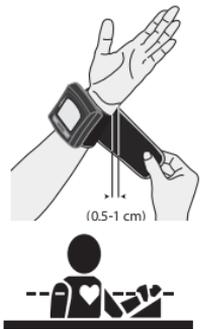

6.4. Measurement Procedure

After the cuff has been appropriately positioned, the measurement can begin:

1. Press the «**ON/OFF**» button. The built-in pump begins to inflate the cuff. In the display, the increasing cuff pressure is continually displayed.
2. After a suitable inflation pressure has been reached, the pump stops and the pressure gradually falls, with cuff pressures being displayed. If that inflation pressure is not sufficient, the monitor automatically re-inflates.
3. When the measurement has been completed, the systolic and diastolic blood pressures and pulse rate now appear in the display.
4. The measurement readings remain on the display until you switch off the instrument. If no button is pressed for a period of two minutes the

instrument switches itself off in order to preserve the batteries.

5. When the unit is set to the MAM setting, three separate measurements will take place in succession, after which your result is calculated and displayed as a single, averaged measurement. There is a 15-second resting time in-between each measurement. A countdown indicates the remaining time.

NOTE: If one of the measurements causes an error message, it will be repeated one more time. If any additional error occurs, the measurement will be discontinued and an error code will be displayed.

Expanding the averaged measurement to see the three individual readings: This function allows you to view the three individual measurements used to calculate the ADC Averaging Mode Technology measurement. **After taking an averaging mode measurement turn unit off, hold the Memory button for three seconds until you hear a short beep. (Do not hold the button longer than seven seconds or you will delete all the readings in the memory!) Let go of the button and watch the screen. It will automatically scroll through the three measurements used in the measurement.**

6.5. Discontinuing a Measurement

If it is necessary to interrupt a blood pressure measurement for any reason (e.g., the patient feels unwell), the «**ON/OFF**» button can be pressed at any time. The device immediately lowers the cuff pressure automatically.

6.6. Reading Measurement Results:

When the measurement has been concluded, the measured systolic and diastolic blood pressure values, as well as the pulse will be displayed.

The appearance of this symbol  signifies that an irregular heartbeat was detected. This indicator is only a caution. It is important that you be relaxed, remain still and do not talk during measurements.

NOTE: We recommend contacting your physician if you see this indicator frequently.

To prolong battery life the device switches off automatically if no button is pressed for two minutes. Otherwise you can switch it off by pressing the «**ON/OFF**» button.

7. SOFTWARE FUNCTIONS (6016N ONLY)

7.1. ADC Advanced PC Link Software Installation and Data Transmission

(Software sold separately, Order Item #6023NPC)

This unit can be used in connection with your personal computer (PC) running the ADC Advanced PC Link Software. Your PC will allow a capacity of monitoring 80 patients, each with 1000 records of data (Note: Overuse will lower system efficiency). The memory data (except average values) can be transferred to the PC by connecting the monitor via the included USB cable with your PC. Note: The software does not work with Mac computers.

- a) Insert CD into CD ROM drive of your PC. The installation will start automatically. If not, click on SETUP.EXE.
- b) Connect the monitor via USB cable with the PC. Three horizontal bars will appear on the display and last for three seconds.
- c) The bars will then flash to indicate that the connection between computer and device is successfully made. As long as the cable is plugged in, the bars will keep flashing and the buttons are disabled. During the connection, the device is completely controlled by the computer. Refer to the 'Help' file in the software for detailed instructions.

Hardware	Minimum	Recommended
Microprocessor (CPU Speed)	550 MHz	1 GHz or higher
Memory devices (RAM)	256 MB	512 MB
Hard disk	500 MB	800 MB
Communications Port	USB 1.0	USB 1.0 and above
Display	256 colors	65536 colors
Resolution	800 x 600	1024 x 760
LPT	available	available
Energy sources (Power supply)	AC power if use PC AC/DC if NB	

Operating System:
Microsoft Window XP, Vista

7.2 Installing and Using Microsoft HealthVault on your ADC Advantage Blood Pressure Monitor

The Advantage Ultra digital blood pressure monitors are compatible with the Microsoft HealthVault software application. HealthVault allows you to easily store, use, and share your health information online and on your mobile devices.

To use HealthVault with your unit, follow the steps below:

1. Create a user account at www.healthvault.com.
2. Once logged in, click on "Apps & Devices."
3. Download the "HealthVault Connection Center" app and follow the prompts on screen to guide you through installation.
4. Once installed, select "Select a Task -> Add Device" from within the HealthVault application.
5. Plug in your ADC BP monitor to your computer using the supplied USB cable. HealthVault will automatically install the device drivers and associate your device to the HealthVault software. At this point, you can start taking readings with your device. Once you have collected a reading, you can now upload the data using the "HealthVault Connection Center" app.
6. Click "Go online to HealthVault" and sign into your account.
7. Click the box of the user you would like to associate with this device and click "Allow Access."
8. Then, click "Upload Now." Your readings will then upload from your device to the HealthVault service.
9. You can then click "View Data in HealthVault" to see your readings.

Once you have approved a device, you will not need to perform these actions again. You can just connect your device and start with step 11.

For more information on how to use HealthVault, click "Help" at the top right-hand corner of the page. There, you will find a detailed help document as well as an FAQ section to help with any issues you may have.

NOTE:

- You cannot run the PC Link software and HealthVault at the same time. Be sure to completely remove the PC Link software before installing HealthVault.
- HealthVault has a mobile app available in both the Apple® App Store and Microsoft® Windows® Phone marketplace.

8. IRREGULAR HEARTBEAT DETECTOR

This function indicates allorhythmic heartbeating. If the symbol of IHD  appears on the display that means that certain abnormalities in heartbeat frequency were detected during the measurement. In this case, the result may deviate from your normal blood pressure – repeat the measurement. In most cases, this is no cause for concern. However, if the symbol  appears on a regular basis (e.g., several times a week with measurements taken daily) we advise you to tell your doctor. Please show your doctor the following explanation:


Information for the doctor on frequent appearance of the Irregular Heartbeat Detector

This instrument is an oscillometric blood pressure monitor that also analyzes pulse frequency during measurement. The instrument is clinically tested. The symbol  is displayed after the measurement, if pulse irregularities occur during measurement. If the symbol appears more frequently (e.g. several times per week on measurements performed daily) we recommend the patient to seek medical advice. The instrument does not replace a cardiac examination, but serves to detect pulse irregularities at an early stage.



8.1. Traffic Light Indicator (6016N only)

The bars on the left hand edge of the display show the range within which the indicated blood pressure values lies. Depending on the height of the bar, the readout value is either within the normal (green), borderline (yellow), or danger (red) range. The classification is based on standards adopted from the WHO (World Health Organization). Refer to the chart here for details of the classification.

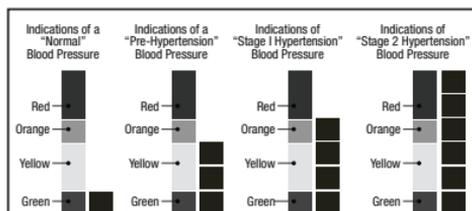

Note: ESH/ESC guidelines may vary from those indicated. Consult your physician for information relating to guidelines in your region.

9. MEMORY FUNCTION

9.1. Recall and Storage of Measurements

At the end of a measurement, this monitor automatically stores each result with date and time. This unit stores 99 memories for each of two users.

Viewing the Stored Values

With the unit off, press the «**MEMORY**» button. The display first shows "A," then shows the average of all measurements stored in the unit.

NOTE: Measurements for each user are averaged and stored separately. Be certain that you are viewing the measurements for the correct user (with no time and date shown).

Pressing the «**MEMORY**» button again displays the previous value. To view a particular stored memory, press and hold the «**MEMORY**» button to scroll to that stored reading.


Further information

Measurements should not occur immediately after each other; otherwise, the results will be skewed. Wait for one minute in a relaxed position, sitting or lying, before you repeat a measurement.

9.2 Delete Memory

Before you delete all memory readings stored, make sure you won't need to refer to them at a later date. Keeping a permanent record is prudent and may provide additional information for your doctor's visit.


To delete stored memory readings, hold the «**MEMORY**» button down until the LCD shows a flashing «**CL**». Release the button. Press the «**MEMORY**» button while «**CL**» is flashing to complete the operation. It is impossible to erase the values individually.



Removing the batteries will also delete the memory.

10. ERROR MESSAGES/TROUBLESHOOTING

If an error occurs during a measurement, the measurement is discontinued and a corresponding error code is displayed (Example: Err 2).



Error No.	Possible Cause(s)/Solutions
ERR 1	Pulse could not be detected. Please ensure the cuff is properly placed on the inside of your wrist and repeat the measurement.
ERR 2	Unnatural pressure impulses influence the measurement result. Reason: the arm was moved during the measurement.
ERR 3	If inflation of the cuff takes too long, the cuff is not correctly seated. Reposition the cuff and repeat the measurement.
ERR 5	The difference between systolic and diastolic is excessive. Measure again carefully following proper procedures. Consult your doctor if you still get unusual results of measurements.
HI	The pressure in the cuff is too high (over 300mmHg). Relax for 5 minutes and repeat the measurement.
LO	The pulse is too low (less than 40 beats per minute). Relax for 5 minutes and repeat the measurement.

Other possible errors and their solutions

If problems occur when using this device, the following points should be checked.

Malfunction	Remedy
The display remains blank when the device is switched on though the batteries are in place.	<ol style="list-style-type: none"> 1. Check battery installation/polarity. 2. Remove the batteries and if the display is unusual, then exchange them for new ones.
The device frequently fails to measure, or the values measured are too low or high.	<ol style="list-style-type: none"> 1. Fit the cuff correctly on the wrist. 2. Before starting measurement make sure that clothing is not exerting pressure on the arm. Take articles of clothing off if necessary. Measure blood pressure again in complete peace and quiet.
Every measurement results in different values, although the device functions normally and normal values are displayed.	Refer to Section 6.2 Common Sources of Error.
Blood pressure values differ from those measured at the doctor's.	Refer to Section 3.7. Why Measure Blood Pressure at Home?

NOTE: Blood pressure is subject to fluctuations even in healthy people. Please remember that **comparable blood pressure measurements always require the same time and the same conditions!**

These are normally quiet conditions. If you follow the procedure described earlier and still get fluctuations of blood pressure of greater than 15 mmHg and/or you repeatedly hear irregular pulse tones, consult your doctor.

Attention!

Should any technical malfunctions arise in the blood pressure monitor, please contact the dealer where you bought the device or ADC. **Never attempt to repair the instrument yourself!** Any unauthorized opening of the instrument invalidates all warranty claims.

11. CARE AND MAINTENANCE

Do not expose the device to either extreme temperatures, humidity, dust or direct sunlight.	
Handle the cuff carefully and avoid all types of stress through twisting or buckling in order not to damage the sensitive air-tight bubble.	
Clean the device with a soft, dry cloth. Do not use gas, thinners or similar solvents. Spots on the cuff can be removed carefully with a damp cloth and soapsuds. Do not submerge the cuff in water!	
Do not drop the monitor or treat it roughly in any way.	
Never open the monitor! This invalidates the manufacturer's warranty.	

Note: According to international standards, your monitor should be checked for calibration every 2 years. Contact ADC for an accuracy check.

12. TECHNICAL SPECIFICATIONS

Weight:	.35 lbs. (148 g) (with batteries + cuff)
Size:	3.75" x 4.25" x 4.25" 85mm x 77mm x 75mm (including cuff)
Storage temperature:	-4 °F – +131 °F / -20 °C – +55 °C
Humidity:	15 to 90% relative maximum humidity
Operation temperature:	50°F–104°F (10°C–40°C)
Display:	LCD (Liquid Crystal Display)
Measuring method:	Oscillometric
Pressure sensor:	Capacitive
Measuring range:	Rated range of the determined - Blood Pressure SYS: 60-255mmHg DIA: 40-200mmHg 40 - 200 beats per minute - pulse
Cuff pressure display range:	0-299 mmHg
Memory:	Automatically stores the last 99 measurements for 2 users (198 total).
Measuring resolution:	1 mmHg
Accuracy:	Pressure within ± 3 mmHg or 2% of the reading ≥ 200 mmHg Pulse ± 5 % of the reading
Power source:	2 AAA batteries
Includes:	Automatic Blood Pressure Monitor with Cuff, 2 AAA batteries, Storage Case, Instruction Book, and Record Book.

13. WARRANTY

This blood pressure monitor is warranted for five years from date of purchase. This warranty includes the instrument and the cuff. The warranty does not apply to damage caused by improper handling, accidents, improper use, or alterations made to the instrument by third parties. The warranty is only valid after the product is registered online at www.adctoday.com.

For Australian Customers: Our goods come with guarantees that cannot be excluded under the Australian Consumer Law. You are entitled to a replacement or refund for a major failure and compensation for any other reasonably foreseeable loss or damage. You are also entitled to have the goods repaired or replaced if the goods fail to be of acceptable quality and the failure does not amount to a major failure.

14. QUALITY STANDARDS

Device standard: This device is manufactured to meet the European and United States standards for non-invasive blood pressure monitors: EN 1060-1/-3/-4; IEC 60601-1-2; ANSI/AAMI/IEC 80601-2-30; ANSI/AAMI/ISO 81060-2

Electromagnetic compatibility: Device fulfills the stipulations of the International standard IEC60601-1-2

Clinical testing: BHS A/A Rated. Clinical performance tests were carried out in the U.K. "Association Protocol and British HTP Protocol."

15. SYMBOL DEFINITIONS

Symbol	Definition
	Important Warning/Caution
	This product is not made with natural rubber latex
	Phthalate free
	Circumference Size
	Meets essential requirements of European Medical Device Directive 93/42/EEC

Symbol	Definition
	Authorized European Representative's Information
	Manufacturer's Information
	Temperature Limit
	Humidity Limitation

16. HOW TO CONTACT US

To register your product and obtain further detailed user information about our products and services visit us at:

www.adctoday.com

and follow the links.

For questions, comments, or suggestions
call us toll free at:

1-800-232-2670



**Onbo Electronic (Shenzhen)
Co., Ltd**

No 138 Huasheng Road, Langkou
Community Dalang Street, Longhua District
Shenzhen, China



Microlife AG

Espenstrasse 139
9443 Widnau/Switzerland



Batteries and electronic devices must be disposed of in accordance with the local applicable regulations, not with domestic waste.



Follow instructions for use. Please read this document thoroughly before using the device and keep for future reference.



Type BF applied part

Dist. by: ADC®
55 Commerce Drive
Hauppauge, NY 11788

Inspected in the U.S.A.

Made in China

tel: 631-273-9600

1-800-232-2670

fax: 631-273-9659

email: info@adctoday.com

www.adctoday.com



0044